

345 Carlingview Drive Toronto, Ontario CANADA M9W 6N9 Tel.: 416.734.3300 Fax.: 416.231.1626 Toll Free: 1.877.682.8772 www.tssa.org

January 24, 2018

SCOTT ISLIP ROUND ENGINEERING INC 10 SEGWUN RD WATERDOWN ON L8B 0K6 CA

Service Request Type.: BPV-National BC Service Request No.: 2180592 Your Reference No.: EH-CRN-27 Registered to.: ENDRESS + HAUSER CONDUCTA INC

Dear SCOTT ISLIP,

Please find enclosed the original response from BC, registered under the CRN No.: 0F19698.51.

As all jurisdictional fees are handled by the Technical Standards and Safety Authority (TSSA), you do not pay any jurisdictions directly.

Should you have any questions or require further assistance, I will be happy to assist you. For general enquiries, please contact a Customer Service Advisor at 1.877.682.TSSA (8772) or e-mail customerservices@tssa.org. When contacting TSSA regarding this file, please refer to the Service Request number provided above.

Yours truly,

Tanya Francis Administrative Assistant_BPV Engineering Tel.: 416-734-3423 Fax: 416-231-6183 Email:tfrancis@tssa.org



505 - 6th Street, Suite 200 New Westminster, BC V3L 0E1

Toll Free: 1-866-566-7233 www.technicalsafetybc.ca

TECHNICAL STANDARDS & SAFETY AUTHORITY 345 CARLINGVIEW DRIVE TORONTO ON M9W 6N9
 Date:
 November 17, 2017

 Account #:
 35231

 Journal #:
 69338

Attn: TANYA FRANCIS

Re: Application for Design Registration

The design, as detailed in your, TSSA SR# 2180592, for a Fitting is accepted for registration as follows:

Registered To: ENDRESS+HAUSER CONDUCTA CRN: 0F19698.51 INC

Drawing #: Report EH-CRN-27

Drawing Revision:0

Conditions Of Registration:

Registration of CONDUMAX CLS16D/CLS16, Hygenic Conductivity Sensor per att'd scope sheets (3 pgs). This design was registered based on a technical review performed by the province of initial registration in accordance with the Association of Chief Inspectors policy on reciprocal recognition of design review.

Reviewer's Notes:

As required by CSA B51 4.2.1, this registration expires on October 03, 2027. This CRN is valid until the expiry date as long as the Manufacturer maintains a valid quality control program verified by an acceptable third-party agency until that date. Should the certification of the quality control program lapse before the expiry date, this registration shall become void.

Contact me if you have any questions. The invoice for registration will be forwarded under separate cover.

SHARON PETERS

boiler.designregistration@technicalsafetybc.ca Design Administration

cc:

ENDRESS+HAUSER CONDUCTA INC.

4123 LA PALMA AVE. ANAHEIM, CA 92807. USA

SCOPE OF CRN REGISTRATION

PRODUCT DESCRIPTION

Description	Design Standard	End Connections	Drawings	EH TI Document
CONDUMAX	ASME B31.3, ASME	1", 1-1/2" and 2" ASME BPE, ISO2852, DIN	414105, 414113, 134267-0002,	
CLS16D/CLS16	B31.1, ASME BPE,	3276 Ferrule (Note 1), DN50 Varivent (Note	134267-0003, 134267-0004, 134267-	TI00227C/07/EN/15.14
	ASME VIII-1 UG-101	1), BioControl D50	0005	

PRESSURE - TEMPERATURE RATINGS

MDMT	MAWP AT 68 F	MAWP AT 248 F	MAWP AT 302 F	NOTES
23F	188 psia	130 psia	87 psia	It is recommended that the sensor be subjected to sterilization at 302F for only a short time (45 minutes approximately)


MATERIALS OF CONSTRUCTION

PROCESS HOUSING MATERIAL (NOTE 2)	SENSOR SHELL MATERIAL	NOTES
STAINLESS STEEL 1.4435 TYPE 316L UNS S31603	POLYPHENYLENE SULFIDE PLASTIC, ASTM A479-316L, STAINLESS STEEL 1.4435 TYPE 316L, UNS S31603, ELASTOMERS	Optional process housing materials may be used. See Note 2.

MANUFACTURING LOCATIONS

Endress+Hauser Conducta	Endress+Hauser Conducta			
70839 Gerlingen incl. manufacturing sites	215021 Suzhou, Endress+Hauser Analytical Instruments Suzhou Co. Ltd.			
04736 Waldheim and 64823 Gross-Umstadt, Germany	P.R. China			
Endress+Hauser Conducta	1 Final CIG Statestiv			
4123 LA Palma Ave., Anaheim, CA	CKINU Annauds& Batery Vessels			
92807, USA	Beinnical Stanue			
4123 LA Palma Ave., Anaheim, CA 92807, USA Note 1) The ASME BPE Ferrule and Varivent connection shall be used with a clamp, however the assembly clamp is not part of this CRN Boilers & Pressure-Temperature ratings may be limited by the clamp type used in the joint assembly. The clamp used to complete the joint shall have Safety Program its own CRN and shall have pressure-temperature ratings the same or higher than the product ratings.				
its own CRN and shall have pressure-temperature ratings the same or higher than the product ratings.				

Note 2) The following additional alloys of superior or equivalent properties to those listed above are also included in the scope of registration: Type 304 S.Steel UNS S30400, Type 304L S.Steel UNS S30403, Type 316 S.Steel UNS S31600, Type 316L S.Steel UNS S31603, Alloy 20 UNS N08020, Hastelloy C-276 UNS N10276, Hastelloy C22 UNS N06022, Hastelloy B3 UNS N10676, Monel 400 UNS N04400 (Note Monel 400 limited to 100F max.), Inconel 600 UNS N06600, Inconel 625 UNS N06625, Inconel 825 UNS N08825, Duplex S.Steel UNS/S318 Super Duplex UNS S32750, Super Duplex UNS S32760, Titanium Grade 3 UNS R50550 (Note Titanium limited to 247F max.)

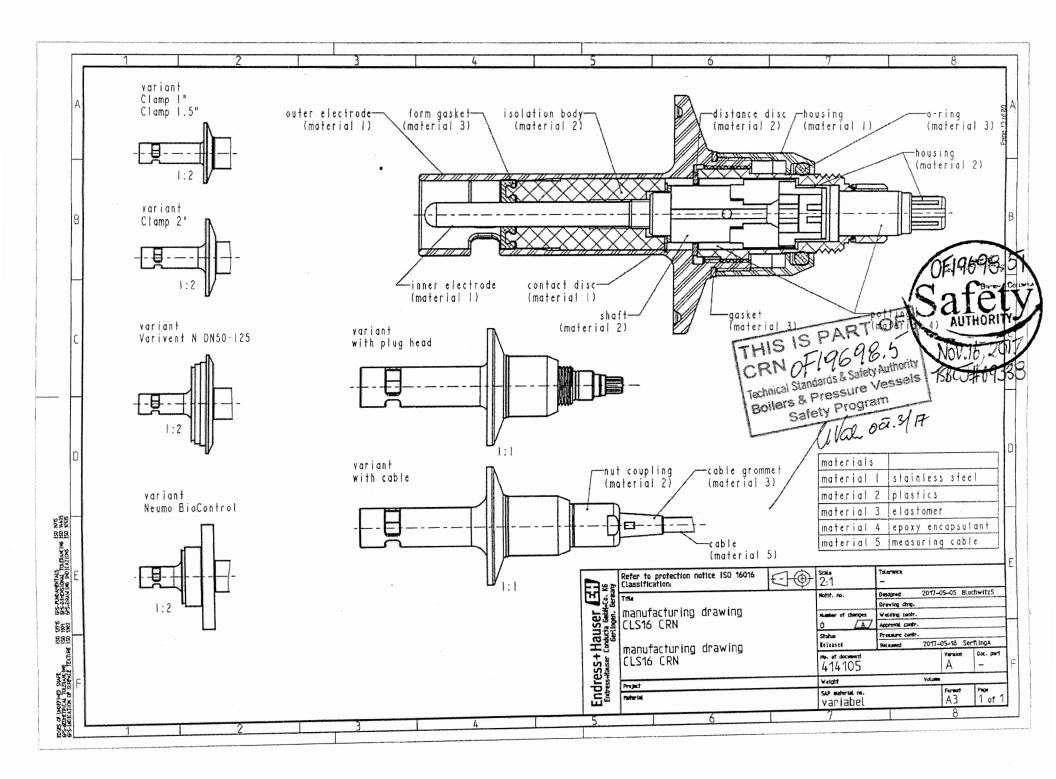

. •. .

